


PCT/IL 02 / 00391



מדינת ישראל
STATE OF ISRAEL

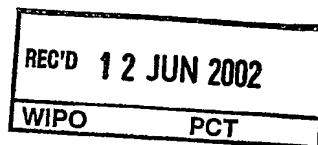

Ministry of Justice
Patent Office

משרד המשפטים
לשכת הפטנטים

This is to certify that
annexed hereto is a true
copy of the documents as
originally deposited with
the patent application
of which particulars are
specified on the first page
of the annex.

זאת לתעודה כי
רצופים בזה העתקים
נכונים של המסמכים
שהופקדו לכתחילה
עם הבקשה לפטנט
לפי הפרטים הרשומים
בעמוד הראשון של
הנספח.

**PRIORITY
DOCUMENT**
SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

This

02-06-2002

היום



נתאשר
Certified

BEST AVAILABLE COPY

לשימוש הלשכה
For Office Use

מספר: Number	143258
תאריך: Date	20-05-2001
הוקדם/נדחה Ante/Post-dated	

חוק הפטנטים, התשכ"ז - 1967
PATENTS LAW, 5727 - 1967

ב ק ש ה ל פ ט נ ט - Application For Patent

אני, (שם המבקש, מענו ולגבי גוף מאוגד - מקום התאגדותו)

I, (Name and address of applicant, and in case of body corporate - place of incorporation)

GIVEN IMAGING LTD.
2 HaCarmel St.
Industrial Park
Yotneam 20692

Israeli Company

גיוון אימגינג בע"מ
פארק התעשיה
רחוב הכרמל 2
יקנעם עילית 20692

חברה ישראלית

בעל אמצאה מכח הדין ששמה הוא
Owner, by virtue of the law of an invention the title of which is

שיטה להדמייה IN VIVO של צינור מערכת העיכול בתנאים שלא שונו

(בעברית)
(Hebrew)

A METHOD FOR INVIVO IMAGING OF THE GASTROINTESTINAL TRACT IN UNMODIFIED
CONDITIONS

(באנגלית)
(English)

בקשת חלוקה - Application of Division	בקשת פטנט מוסף - Application for Patent Addition	דרישה דין קדימה Priority Claim		
מבקשת פטנט from Application	לבקשה/לפטנט to Patent/Appl.	מספר/סימן Number/Mark	תאריך Date	מדינת האגוד Convention Country
No..... מס'..... dated..... מיום.....	No..... מס'..... dated..... מיום.....			
יפוי-כח: POA: הוגש בענין P.A. 108352 המען למסירת מסמכים בישראל Address for Service in Israel איתן, פרל, לצר וכהן-צדק עורכי דין, עורכי פטנטים ונוטריון רח' שנקר 7, הרצליה 46725		היום 20 לחודש מאי שנת 2001 This 20 of May of the year 2001		
חתימת המבקש Signature of the Applicant עבור המבקש, For the Applicant, איתן, פרל, לצר וכהן-צדק EITAN, PEARL, LATZER & COHEN-ZEDEK P-4165-IL		לשימוש הלשכה For Official Use		

טופס זה, כשהוא מוטבע בחותם לשכת הפטנטים ומושלם במספר ובתאריך ההגשה, הנו אישור להגשת הבקשה שפרטיה רשומים לעיל.
This form, Impressed with the Seal of the Patent Office and indicating the number and date of filing, certifies the filing of the application the particulars of which are set out above.

* מחק את המיותר Delete whatever is inapplicable

**A METHOD FOR IN VIVO IMAGING OF THE
GASTROINTESTINAL TRACT IN UNMODIFIED CONDITIONS**

שיטה להדמייה IN VIVO של צינור מערכת העיכול בתנאים שלא שונו

Eitan, Pearl, Latzer & Cohen-Zedek

P-4165-IL

A METHOD FOR IN VIVO IMAGING OF THE GASTROINTESTINAL TRACT IN UNMODIFIED CONDITIONS

FIELD OF THE INVENTION

The present invention relates to in vivo imaging of the digestive tract. Specifically, the invention relates to in vivo imaging of the gastrointestinal tract in unmodified conditions.

BACKGROUND OF THE INVENTION

Endoscopes for visual examination of body lumens usually include a flexible tube inserted into the body lumen. The tube usually includes a remote illumination source which delivers illumination through an optical fiber, and an imaging camera, typically including a lens and an imager (CCD or CMOS).

Figure 1 schematically illustrates a prior art endoscope. In the endoscope 10, the illumination source 12 is located along side the camera 13 and camera lens 14, resulting in only partial overlapping between the field of illumination 112 and the field of view 114. Usually the non-overlapping area between the two fields is small and not significant.

Figure 2A schematically illustrates a prior art endoscope 20 inserted into the intestine 26 (e.g. the small intestine). The field of illumination 222 and field of view 224 overlap enabling acquisition of images from the intestine 26.

Figure 2B schematically illustrates a prior art endoscope 20 inserted into the intestine 26 when the field of illumination 222 is obscured by a fold of the intestine 26' or by the intestine wall collapsing on the tip of the endoscope 20. In this case there is no overlapping between the field of illumination 222 and the field of view 224 and acquisition of images of the intestine is prevented. Also, the obscuring of the field of view 224 by the fold in the intestine wall 26' is enough to prevent image acquisition.

The problem of obscuring of the tip of the endoscope, as described above, is well known in the art and is usually solved by insufflating air in the intestine. Figure 3 schematically illustrates a prior art endoscope 30 in an air insufflated intestine 36. Air insufflation inflates the intestinal walls, flattens the folds that are naturally present in the intestine wall, and removes potential obstruction from both the illumination source 34 (field of illumination 304) and from the lens 32 (field of view 302).

Air insufflation of the intestine, although solving problems of optical obstruction, changes the normal physiological conditions of the intestine. Under normal physiological conditions the intestine is collapsed and most of the remaining space is filled with the gastrointestinal liquid. Under insufflation the intestine is filled with air leaving the liquid spread as a moisture layer only on the intestinal wall. In an unmodified environment viewing conditions in the intestine are similar to underwater viewing. Air insufflation modifies these conditions possibly leading to degradation of some colors seen through the air (similar to tropical fishes which have vivid colors in the water but pale colors once the fish is in the air).

P-4165-IL

In addition to differences in geometry and in the physics of viewing the intestine under modified and unmodified conditions, physiological differences may develop due to insufflation and the resulting air pressure in the intestine.

For example, a tamponade effect results in increased pressure on small blood vessels possibly resulting in stopping any existing bleeding. Thus, effective detection of bleeding sites in the gastrointestinal (GI) may be prevented. Also, villi collapse in the air diminishing the quality of obtained images, as compared to villi floating in the gastrointestinal liquid. Further, in rare cases fatal air embolism may occur as a result of insufflation endoscopy (Katgraber F, Glenewinkel F, Fischler S, *Int J Legal Med* 1998; 111(3) 154-6.).

SUMMARY OF THE INVENTION

The present invention provides a method and device for in vivo imaging of the gastrointestinal tract in unmodified conditions, namely under natural physiological conditions, in which obscuring of the field of view or of the field of illumination is prevented.

The invention is based on viewing the intestine through an optical dome which prevents obscuring of the field of illumination or of the field of view, due to collapse or due to a fold of the intestine wall. The invention also enables to obtain in vivo images of the gastrointestinal tract having a quality that is not impaired by modifications of the intestinal environment, such as by insufflation.

The method of the present invention includes the steps of: introducing into an uninsufflated intestine an imaging device for imaging the uninsufflated intestine, and obtaining images of the uninsufflated intestine. The imaging device comprises at least one dome shaped or convex end through which the uninsufflated intestine is illuminated and viewed.

The present invention further provides a method for viewing submucosal formations in the intestine. The method includes the steps of: introducing into an uninsufflated intestine an imaging device for imaging the uninsufflated intestine; illuminating collapsed walls of the intestine; obtaining images of the collapsed intestine walls; and obtaining from the images of the collapsed intestine wall a view of submucosal formations of the intestine. The imaging device comprises at

P-4165-IL

least one dome shaped or convex end through which the uninsufflated intestine is illuminated and viewed.

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention will be understood and appreciated more fully from the following detailed description taken in conjunction with the drawings in which:

Figure 1 is a schematic illustration of a prior art endoscope;

Figure 2A and 2B are schematic illustrations of a prior art endoscope in a gastrointestinal tract (2A) and in a portion of the gastrointestinal tract having a fold (2B);

Figure 3 is a schematic illustration of a prior art endoscope in an insufflated intestine;

Figure 4 is a schematic illustration of an in vivo imaging device in an intestine with unmodified environment, in accordance with an embodiment of the invention;

Figure 5 is a schematic illustration comparing the illumination of a prior art endoscope in an insufflated intestine with the illumination of an in vivo imaging device according to an embodiment of the invention;

Figure 6 is a schematic illustration comparing the optical path of a prior art endoscope in an insufflated intestine with the optical path of an in vivo imaging device according to an embodiment of the invention;

Figure 7 schematically illustrates an angular resolution scheme for air-insufflated endoscopy and for endoscopy in accordance with an embodiment of the invention;

P-4165-IL

Figure 8 is a more detailed, three-dimensional scheme of the schematic illustration of Figure 7; and

Figures 9 and 10 present angular resolution and apparent magnification for air-insufflated endoscopy and for endoscopy in accordance with an embodiment of the invention.

DETAILED DESCRIPTION OF THE INVENTION

In the following discussion, present invention will be also referred to as "airless endoscopy".

Reference is now made to Fig. 4 which presents a schematic illustration of an in vivo imaging device, specifically designed, in accordance with the invention, to view the gastrointestinal tract in an unmodified environment. The in vivo imaging device 40 is a device capable of being inserted and moved through the intestine, such as an endoscope. The dome or convex shaped tip 402 of endoscope 400 is an optical window 42 through which the intestine is illuminated and viewed and/or imaged. One or more illumination sources 46 and an imager and lens 44 are positioned behind optical window 42. The collapsed, uninsufflated intestine walls 410 are in close proximity to the imaging device 40 and present only a limited area 412 to be viewed. In these conditions the field of view 404 includes the entire area 412. Furthermore, illumination field (or fields) 406 provided by illumination sources 46 illuminate the entire area 412. Hence, at any point of time during the imaging device's 40 progress through the intestine a limited area of the intestine wall is fully illuminated and can be viewed in its entirety. As imaging device 40 progresses along the intestine it can collect full images of the entire gastrointestinal tract.

As will be shown and discussed below, an imaging device designed in accordance with the invention operates more efficiently than prior art imaging devices operating in insufflation conditions to obtain images that are of an

improved quality compared to images obtained under insufflation conditions. Furthermore, these images contain information that is unobtainable under insufflation conditions of the intestine.

As is shown in Fig. 5 the illumination efficiency of imaging device 50, designed in accordance with the invention, is higher than that of prior art imaging device 51. Illumination angle α is not as sharp an angle compared with sharp illumination angle β , such that most of the illumination is efficient and is returned by the intestine wall back to the imaging device and lens 52.

As shown in Fig. 6 also the viewing angle of the device in accordance with the invention is less sharp than the viewing angle of a prior art imaging device. Therefore, formations such as arterioles, venules, lymphatic ducts and others which are located submucosally are viewed through a thinner layer of mucosa than while using a prior art imaging device. As can be seen in Fig. 6 the optical path to the submucosal formation 604 is shorter (see distance v-w) when using an imaging device 60 in accordance with the invention than when using a prior art imaging device 61 (see distance v'-w').

Due to different geometry of the two techniques, their spatial resolution is also different. Fig. 7 presents a simplified planar scheme for calculation of angular resolution and apparent magnification. Fig. 8 presents a more detailed, three-dimensional scheme. Figs. 9 and 10 present angular resolution and apparent magnification for air insufflating and airless endoscopy. It can be understood that airless endoscopy provides superior resolution in most angles of the field of view. For the simplicity of discussion we will make several assumptions: Insufflation causes the intestine to be cylindrical shaped with radius R2. Endoscopic optical axis aligns with the geometrical axis of the intestine.

P-4165-IL

In the airless endoscopy collapsed walls of the intestine form a half-sphere around the optical dome of the endoscope. Radius half a sphere is R_1 . Both cases are shown in Fig. 7. It should be noted that usually $R_1 < R_2$.

Finding angular resolution

The objective is to find what will be the angles $\Delta\theta$ and $\Delta\varphi$ (along the two orthogonal axis) for an object that has length of ΔL_θ (or ΔL_φ) as function of the view angle θ (or φ) correspondingly.

Case 1. Air insufflating endoscopy.

a. Angle (axis) θ

$$L_\theta = R_2 * \text{ctg } \theta$$

$$dL_\theta/d\theta = R_2 * (-1/\sin^2\theta)$$

It should be noted that only an absolute value of the expression is important, therefore the minus sign will be omitted.

b. Angle (axis) φ

$$L_\varphi = (R_2/\sin\theta) * \text{tg } \varphi$$

$$dL_\varphi/d\varphi = (R_2/\sin\theta) * (1/\cos^2\varphi)$$

Case 2. Airless endoscopy.

a. Angle (axis) θ

$$L_\theta = R_1 * \theta$$

$$dL_\theta/d\theta = R_1$$

b. Angle (axis) φ

P-4165-IL

$$L_{\varphi} = R_1 * \varphi$$

$$dL_{\varphi}/d\varphi = R_1$$

Assuming $R_1=R_2$ the normalized (relative) angular resolution of both methods may be calculated. Figure 8 presents results of the calculation (in order to make the visual presentation more illustrative, inverse value is plotted: $d\theta/dL$

Angular resolution of the airless endoscopy is better, especially for low values of the viewing angles.

Finding apparent magnification.

Figure 9 shows geometrical relations used for calculation of linear resolution (apparent magnification), for air insufflation, and for airless endoscopy.

Magnification is defined as a ratio between the size of the object on the imager and actual size of the object. It may be defined without units or with units, e.g. [pixel/meter].

Angular resolution [m/?] versus view angle for air insufflating endoscopy. The line referred to as line 90 describes resolution versus θ . Other lines describe resolution versus φ (angle θ serves here as a parameter). Angular resolution in airless endoscopy does not depend on the viewing angle and is 1, assuming the same diameter of the intestine ($R_1=R_2$). Difference in the resolution is increases assuming that the insufflation increases diameter of the intestine ($R_1 < R_2$).

Case 1. Air insufflating endoscopy.

a. Angle (axis) θ

$$\operatorname{tg}\theta = L_{\theta}/F = R_2/L_{\theta}$$

$$L_{\theta} = R_2/\operatorname{tg}\theta$$

From here we can express through θ :

$$L_{\theta} = F \cdot R_2 / L_{\theta} = F / \operatorname{tg}\theta$$

Derivative will show the linear resolution:

$$DL'_{\theta}/dL_{\theta} = -R_2 \cdot F / L_{\theta}^2 = -R_2 \cdot F / (R_2^2/\operatorname{tg}^2\theta) = -F/R_2 \cdot \operatorname{tg}^2\theta$$

b. Angle (axis) φ

$$L'_{\varphi} = F/\cos\theta \cdot \operatorname{tg}\varphi$$

$$L_{\varphi} = R_2/\sin\theta \cdot \operatorname{tg}\varphi$$

$$L'_{\varphi} = F/\cos\theta \cdot (\sin\theta/R_2) \cdot L_{\varphi} = F/R_2 \cdot \operatorname{tg}\theta \cdot L_{\varphi}$$

$$dL'_{\varphi}/dL_{\varphi} = F/R_2 \cdot \operatorname{tg}\theta$$

Case 2. Airless endoscopy.

a. Angle (axis) θ

$$L'_{\theta} = (F \cdot \operatorname{tg}\theta/R_1 \cdot \theta) \cdot L_{\theta}$$

$$dL'_{\theta}/dL_{\theta} = F \cdot \operatorname{tg}\theta/R_1 \cdot \theta$$

b. Angle (axis) φ

$$L'_{\varphi} = (F/R_1 \cdot \operatorname{tg}\varphi/\varphi \cdot 1/\cos\theta) \cdot L_{\varphi}$$

$$dL'_{\varphi}/dL_{\varphi} = F/R_1 * \tan \varphi / \cos \theta$$

Magnification for different viewing angles is shown in Figure 10. In Fig. 10 Magnification [pixels/meter] versus view angle for air insufflating endoscopy is compared to airless endoscopy (assuming same diameter of the intestine). For airless endoscopy magnification versus θ is shown, and magnification versus φ is shown, while θ is a parameter: $\theta = 10^\circ$ $\theta = 45^\circ$ $\theta = 70^\circ$. For air insufflating endoscopy magnification versus θ and φ is shown. It may be seen that magnification (resolution) of airless endoscopy is superior, especially in central area. Assuming that the insufflation increases diameter of the intestine ($R_1 < R_2$) —performance of the airless endoscopy is improved.

It may be concluded that linear resolution of airless endoscopy is superior to air insufflating endoscopy in most angles of the field of view. Figure 10 presents the case when diameter of the intestine is the same in the air-insufflating and airless endoscopy ($R_1 = R_2$). It is a reasonable assumption the air insufflation increases diameter of the intestine ($R_1 > R_2$). Therefore linear resolution in the air-insufflating case will have even lower values than that presented in Figure 10.

It will be appreciated by persons skilled in the art that the present invention is not limited to what has been particularly shown and described hereinabove. Rather the scope of the present invention is defined only by the claims which follow:

CLAIMS

1. A method for in vivo imaging of the gastrointestinal tract in unmodified conditions comprising the steps of:
 - introducing into an unsufflated intestine an imaging device, said
 - imaging device comprising at least one convex end through which the
 - unsufflated intestine is illuminated and viewed; and
 - obtaining images of the unsufflated intestine.

2. A method for viewing submucosal formations in a patient's intestine, said method comprising the steps of:
 - introducing into an unsufflated intestine an imaging device, said
 - imaging device comprising at least one dome shaped or convex end
 - through which the unsufflated intestine is illuminated and viewed;
 - illuminating collapsed walls of the intestine;
 - obtaining images of the collapsed intestine walls; and
 - obtaining from the images of the collapsed intestine wall a view
 - of submucosal formations of the intestine.

3. An imaging device in vivo imaging of the gastrointestinal tract in unmodified conditions, said imaging device comprising at least one convex end through which the intestine is illuminated and viewed.

P-4165-IL

4. An imaging device according to claim 3 wherein the unmodified conditions
comprise an unsufflated intestinal environment.

For the Applicant

Rachel Bentor

Eitan, Pearl, Latzer & Cohen Zedek
Advocates, Patent Attorneys & Notaries
P-4165-IL

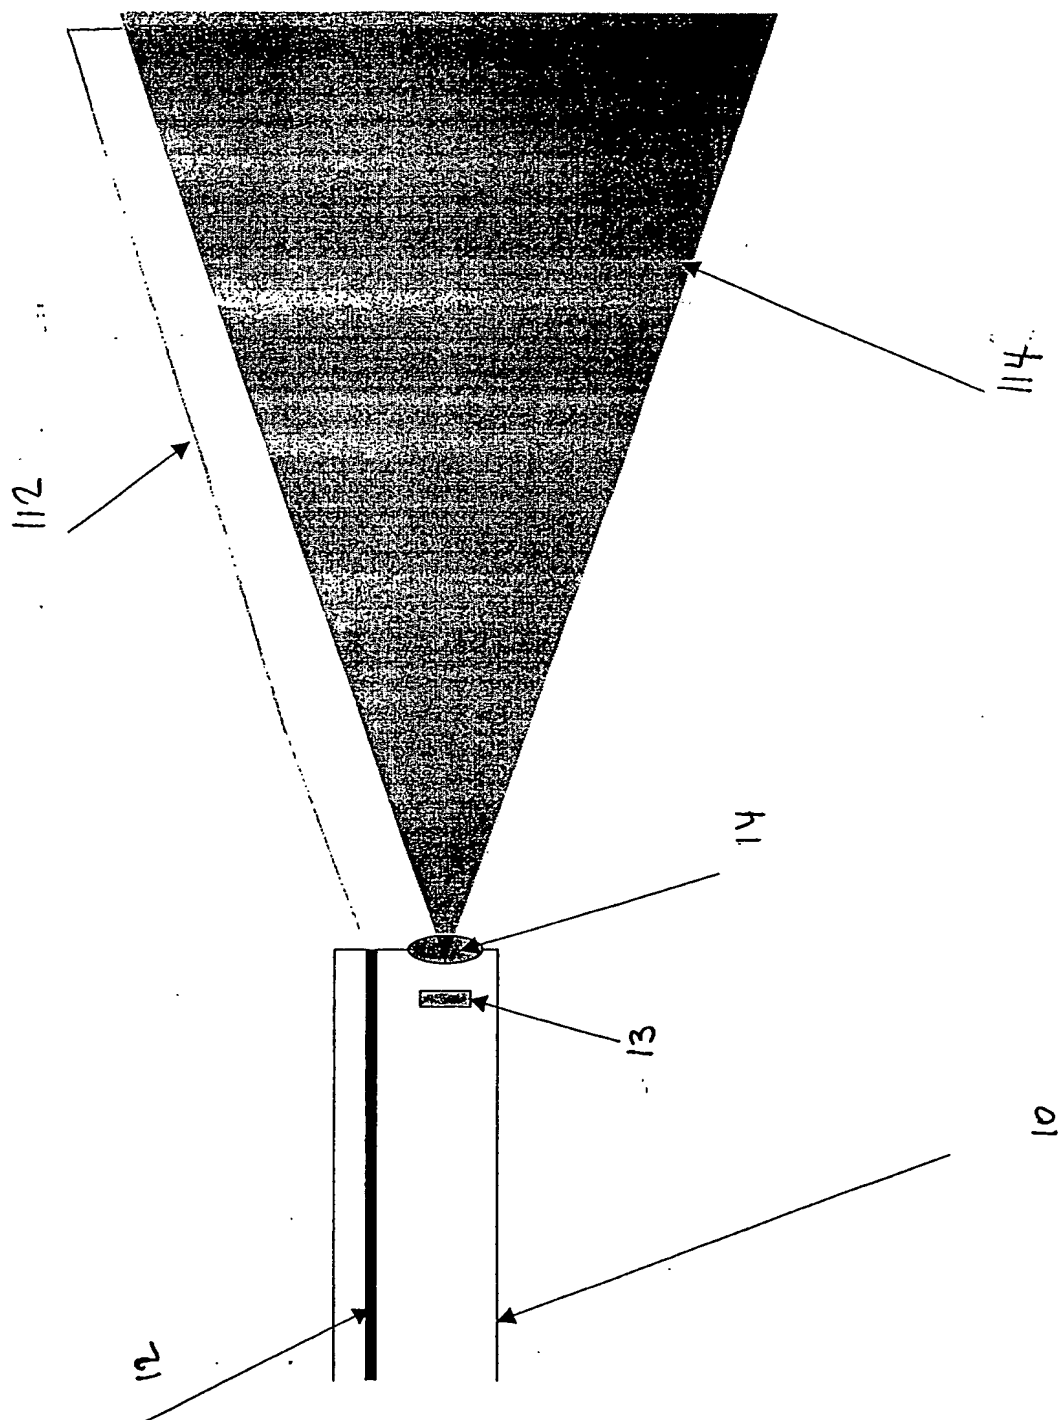


Figure 1
PRIOR ART

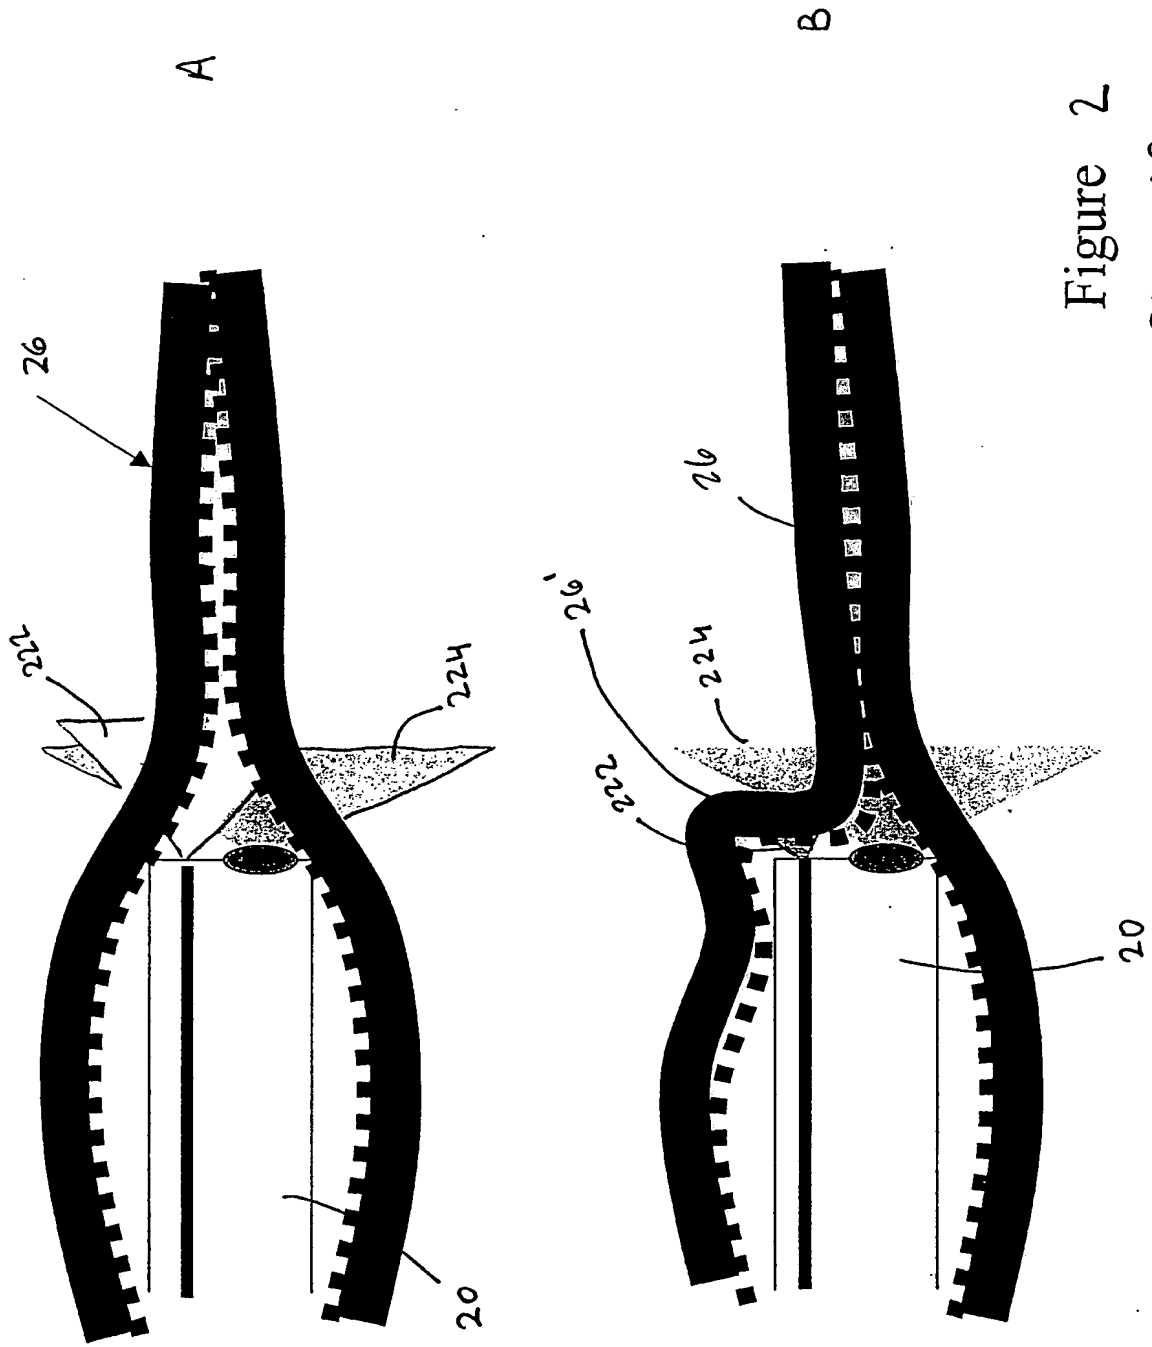


Figure 2
PRIOR ART

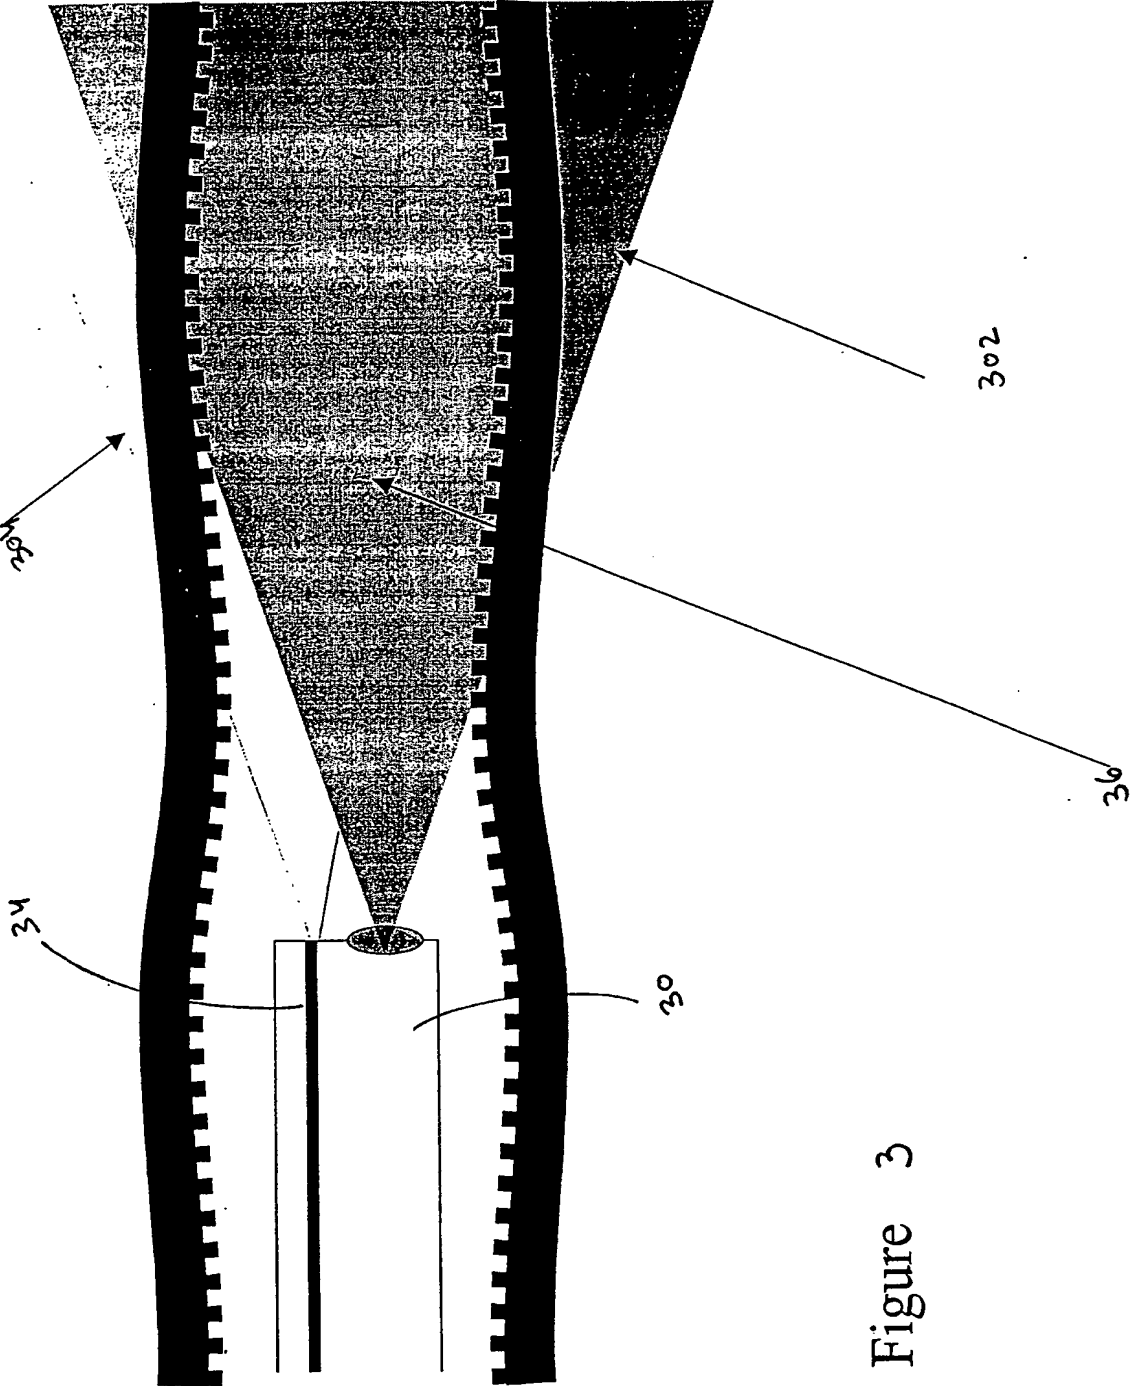


Figure 3

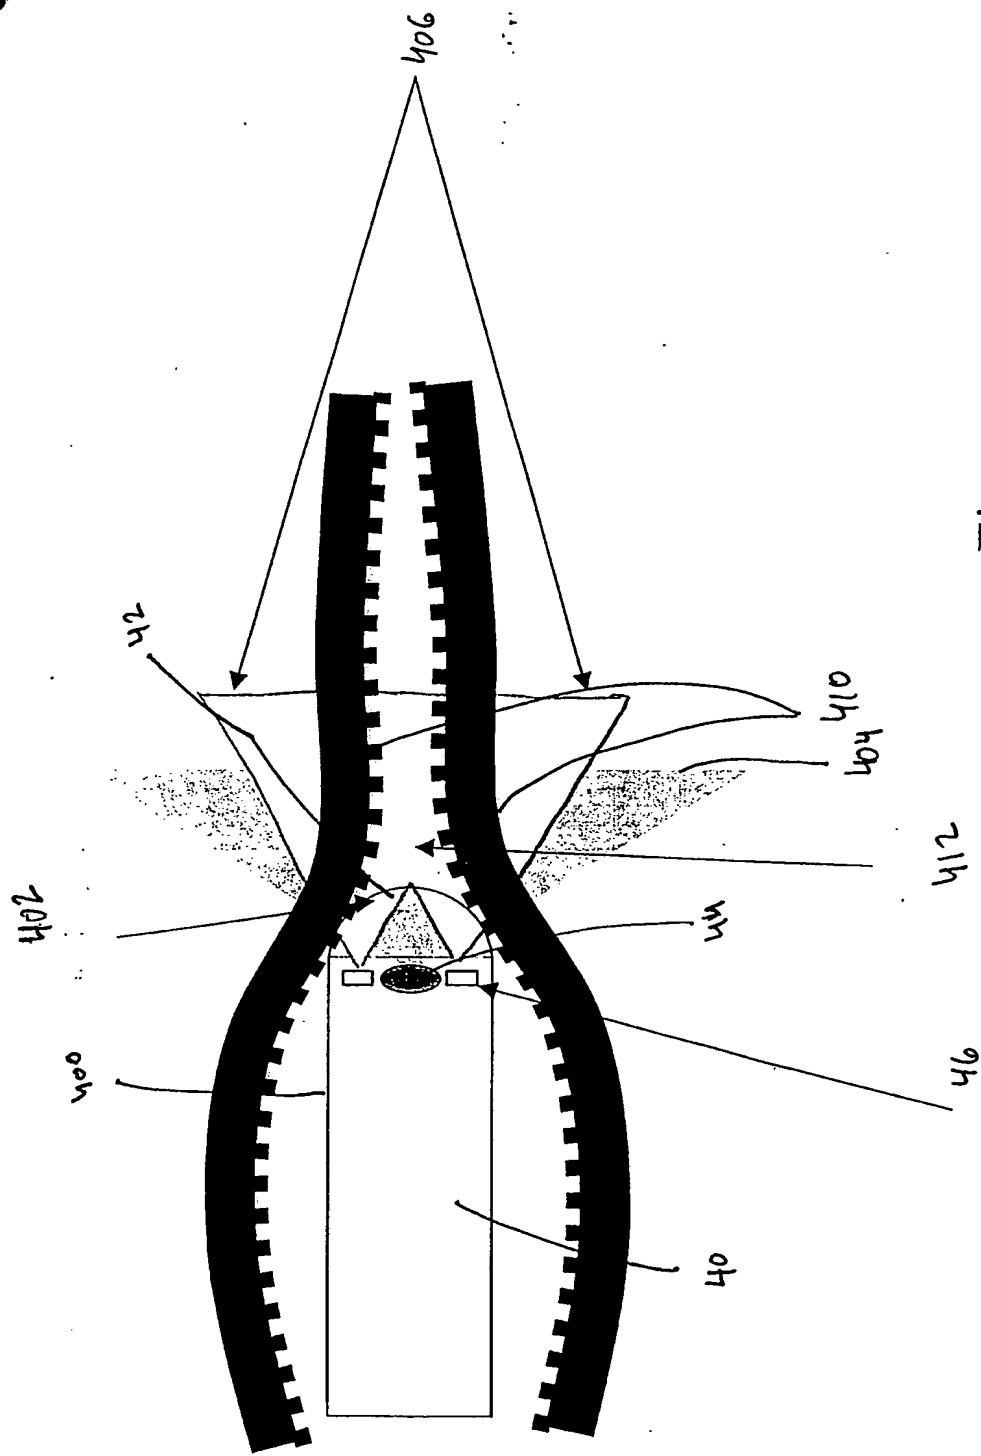


Figure 4

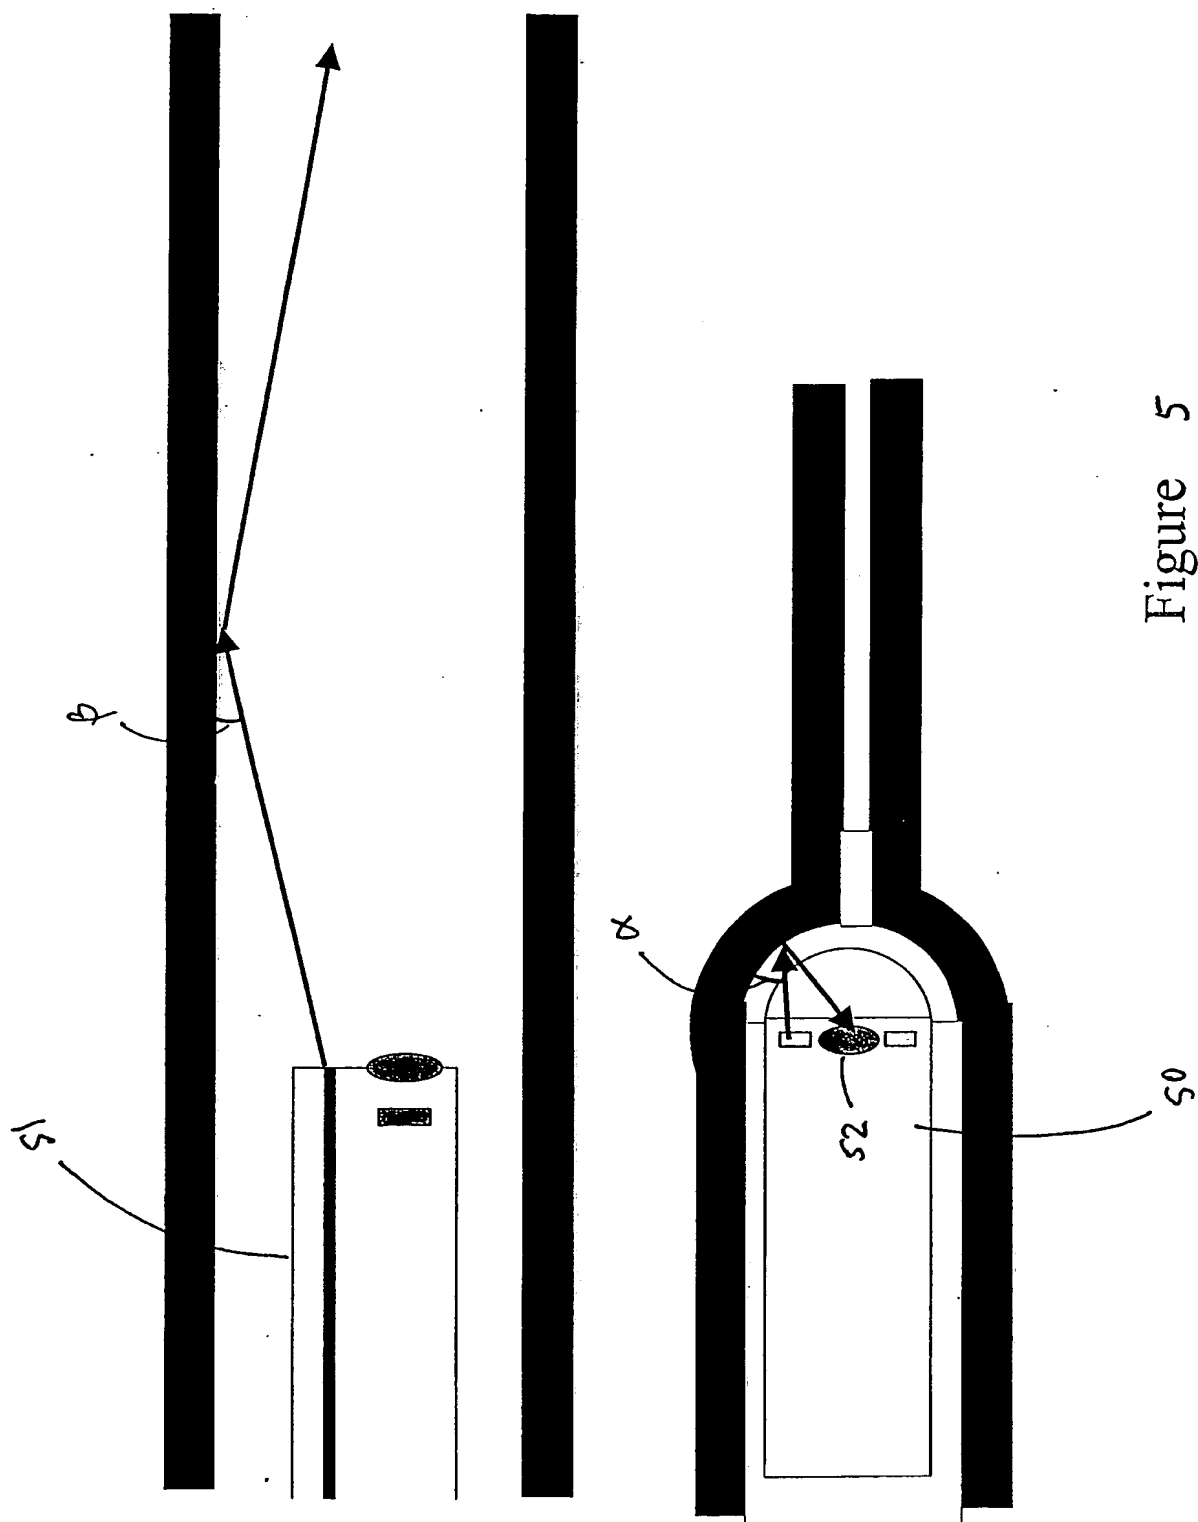
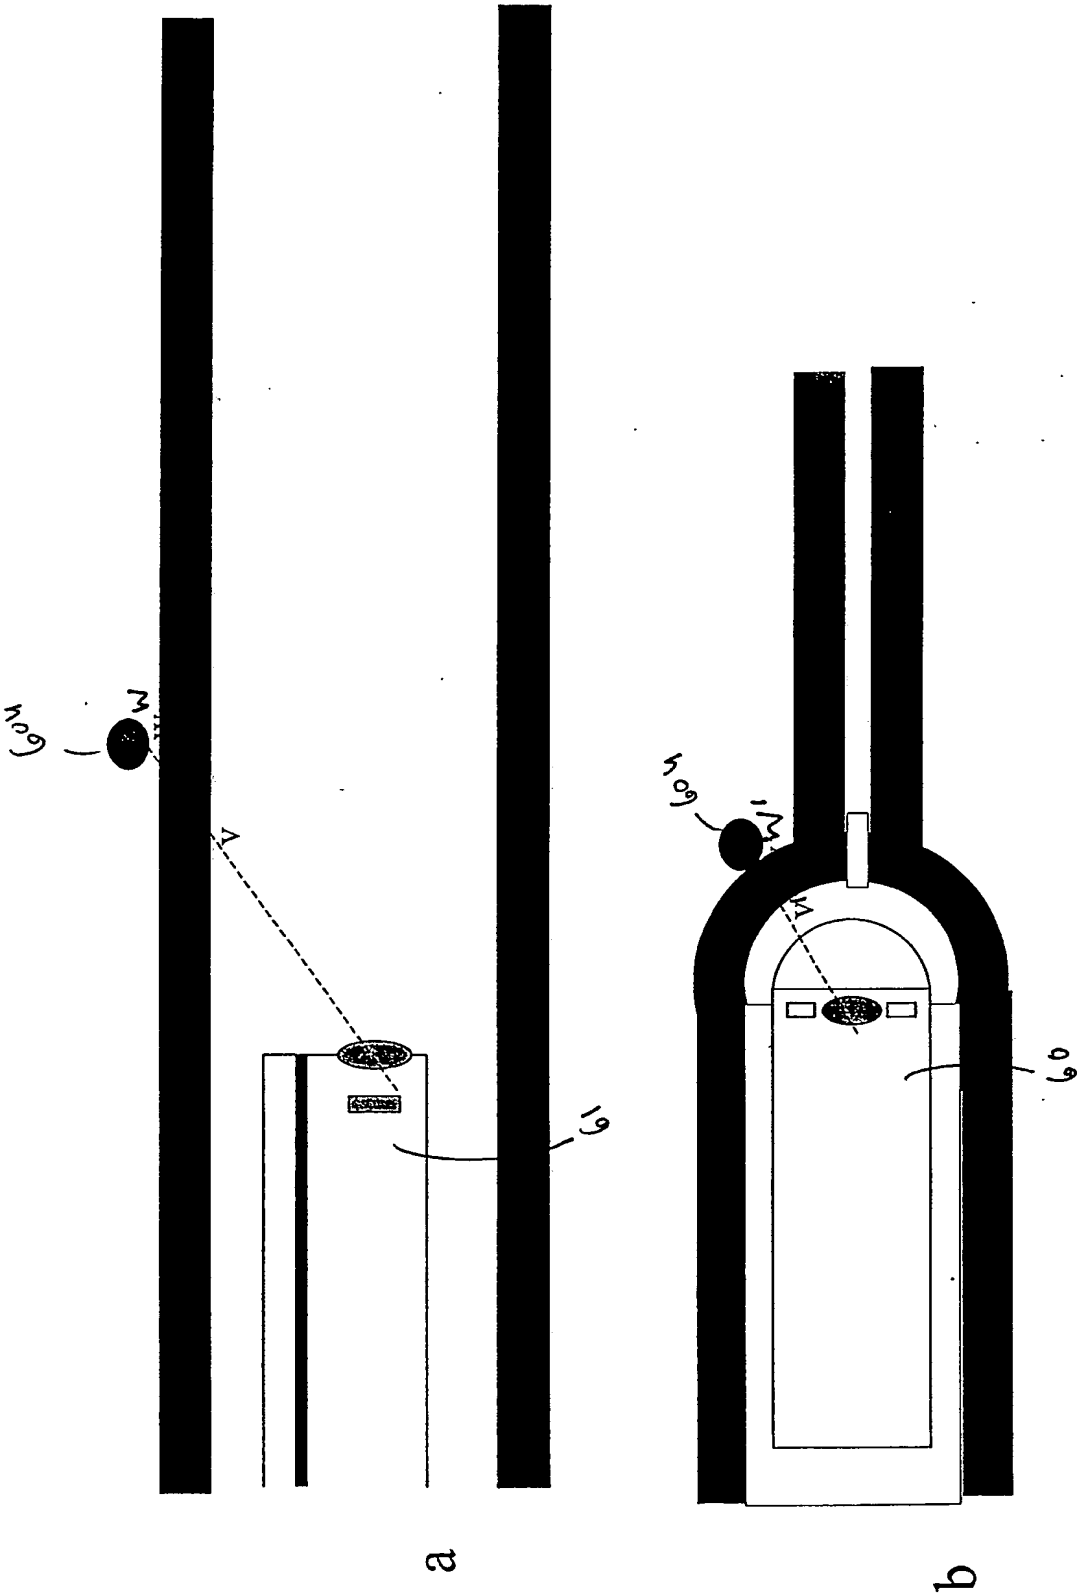


Figure 5

Figure 6



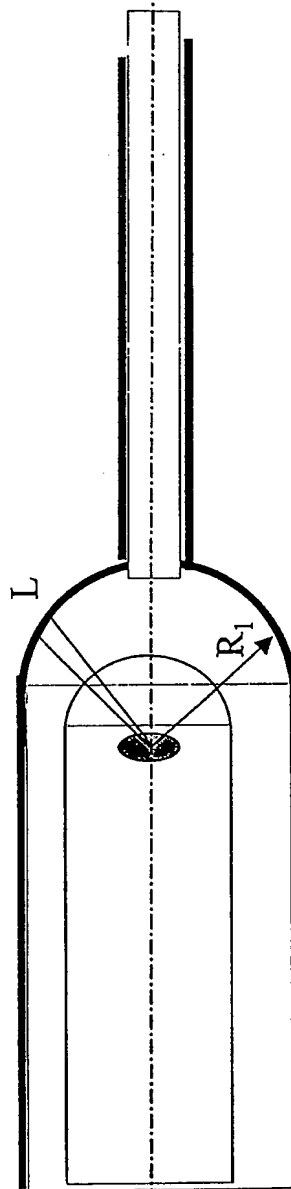
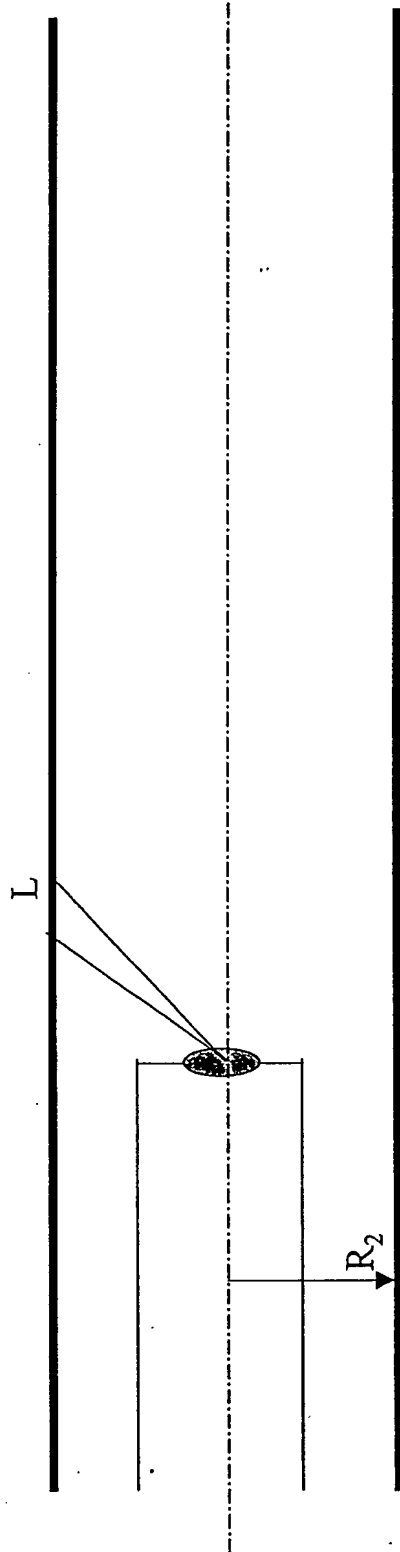


Figure 7

Figure 8

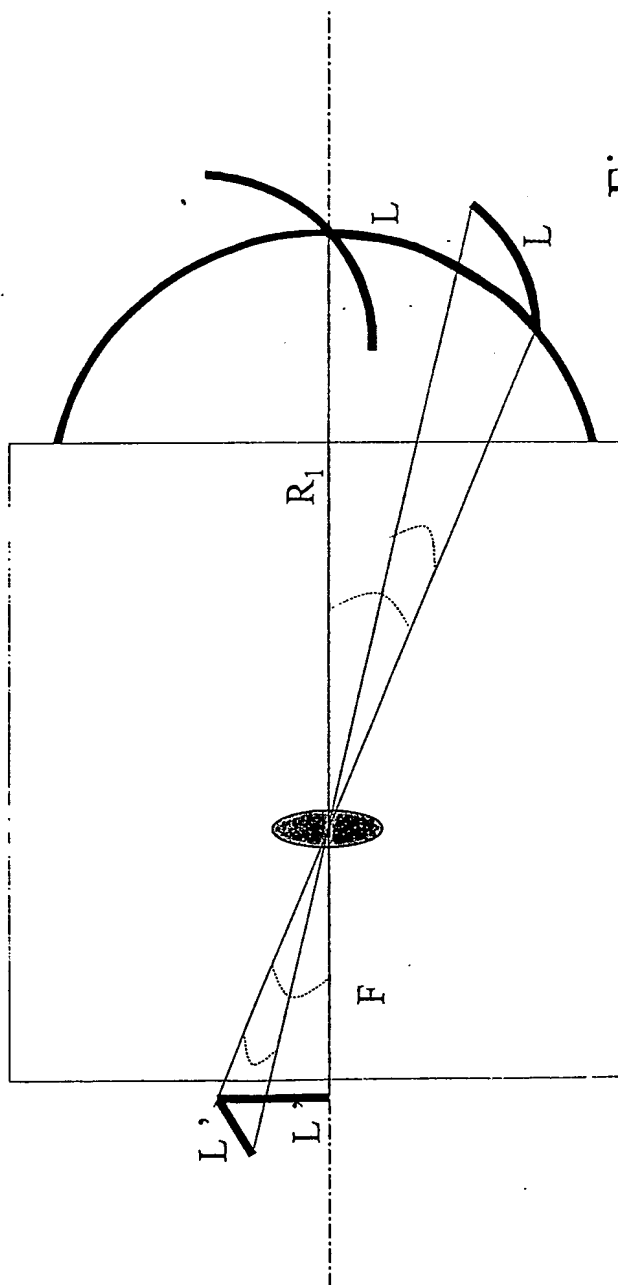
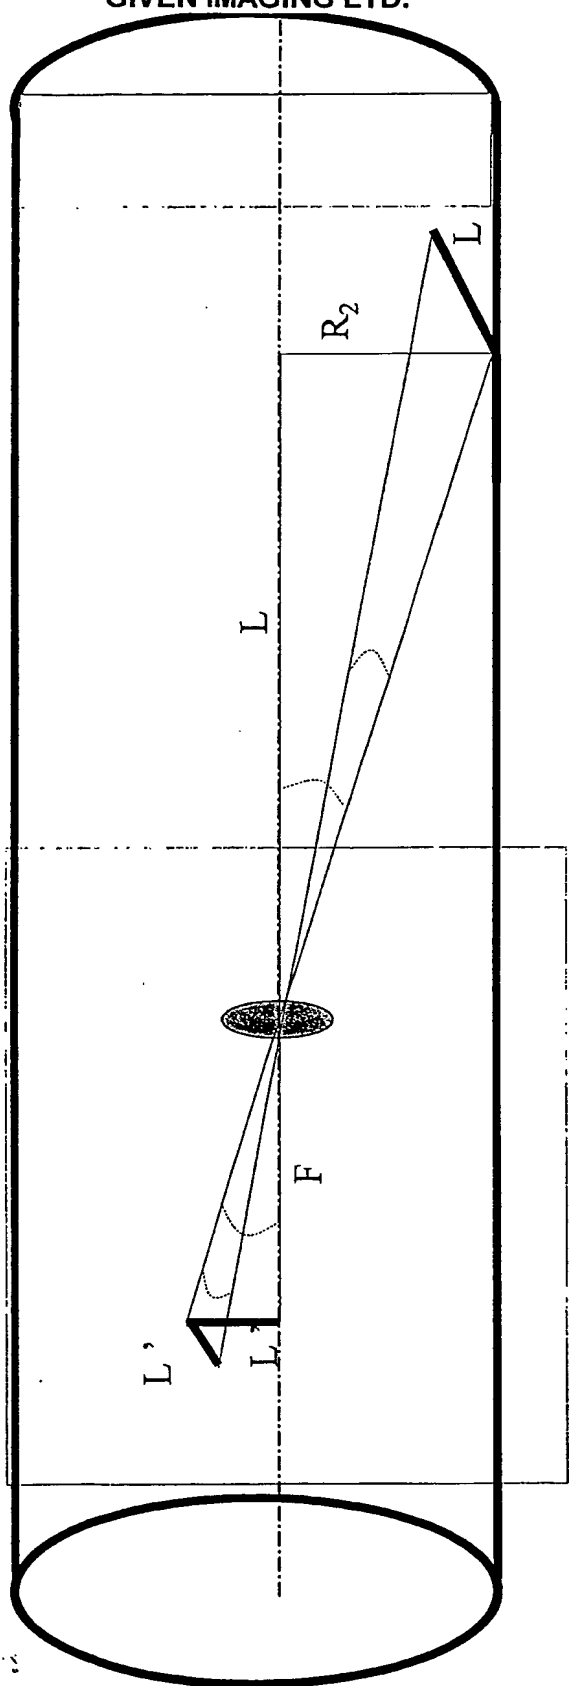
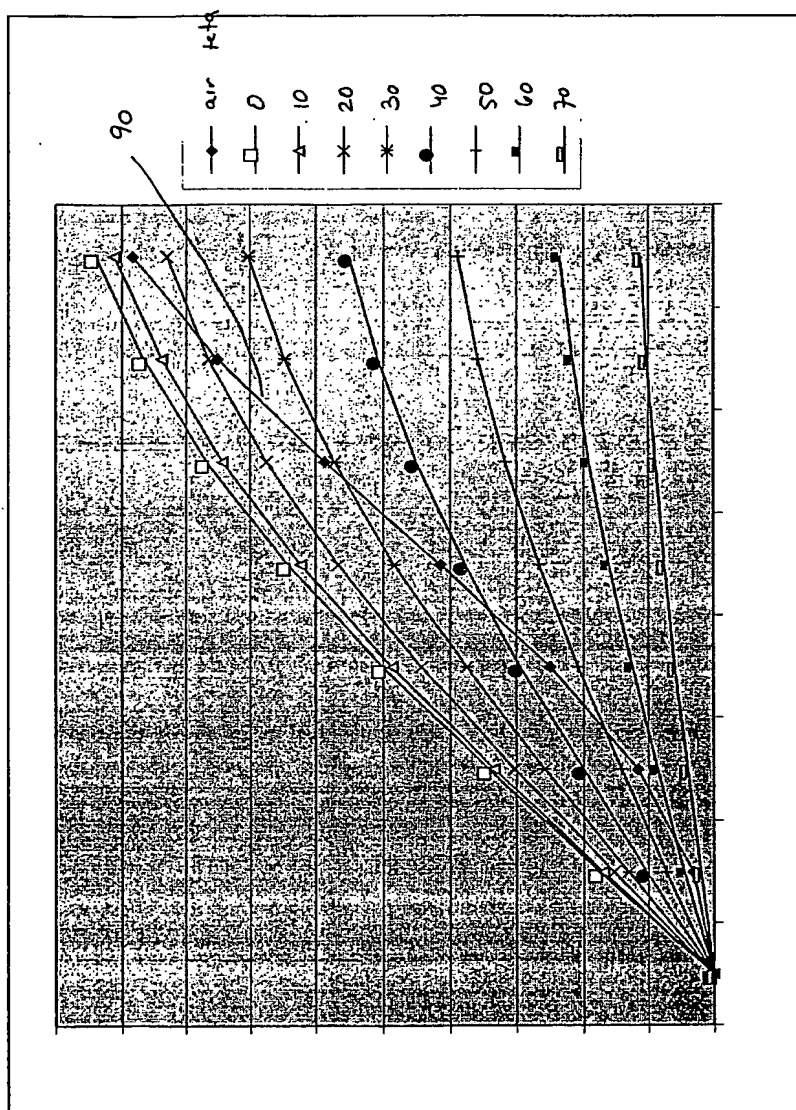


Figure 9



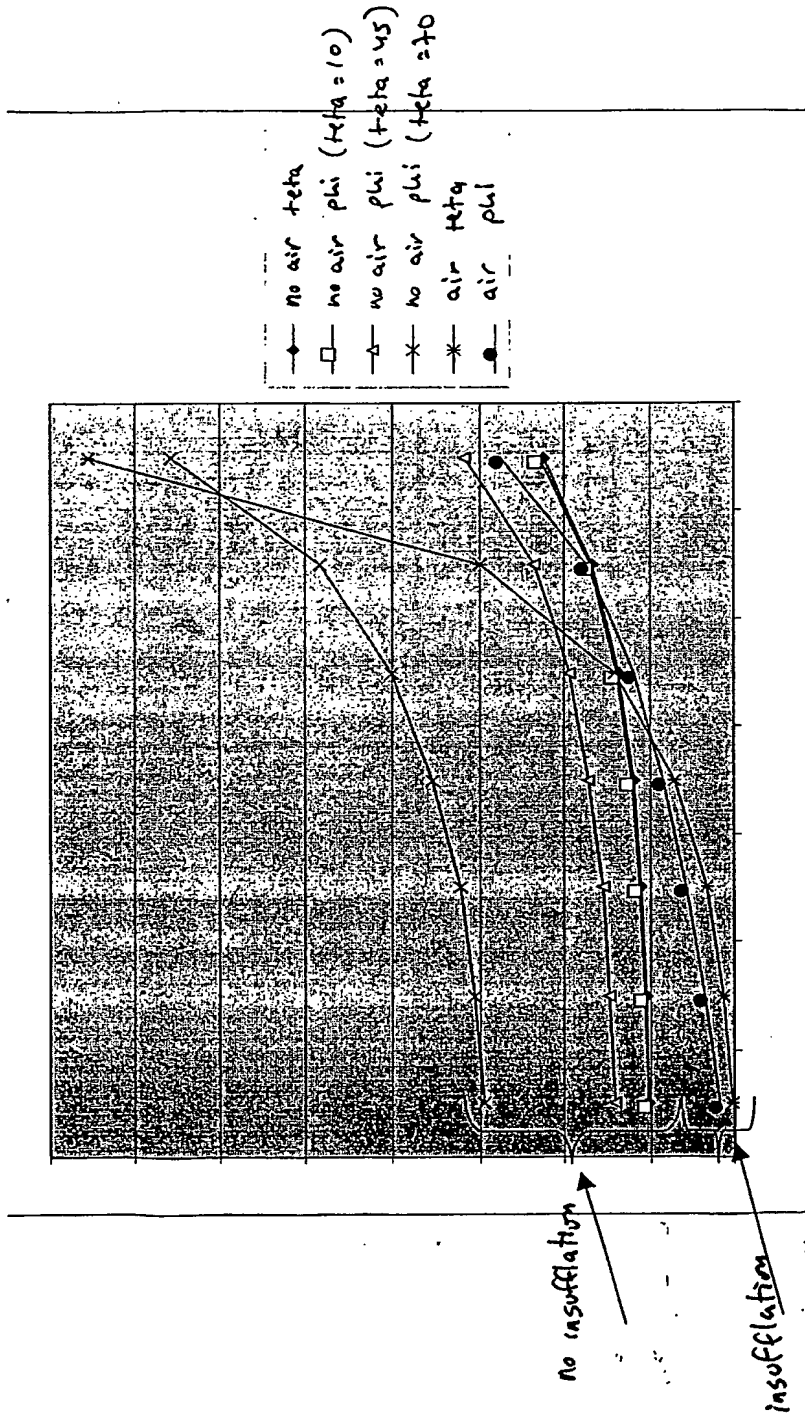


FIGURE 10

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

☒ BLACK BORDERS

☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES

☒ FADED TEXT OR DRAWING

☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING

☐ SKEWED/SLANTED IMAGES

☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS

☐ GRAY SCALE DOCUMENTS

☐ LINES OR MARKS ON ORIGINAL DOCUMENT

☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY

☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.